


+ technical operation



+ optional

- Integrated barcode reader to read the serial number of endoscopes and operators and related traceability of the executed cycles downloading data from USB port (already equipped with 50 instrument acid-resistant barcode labels and 20 for operators).
- Olympus, Pentax, Fujinon and Storz leak test connectors.

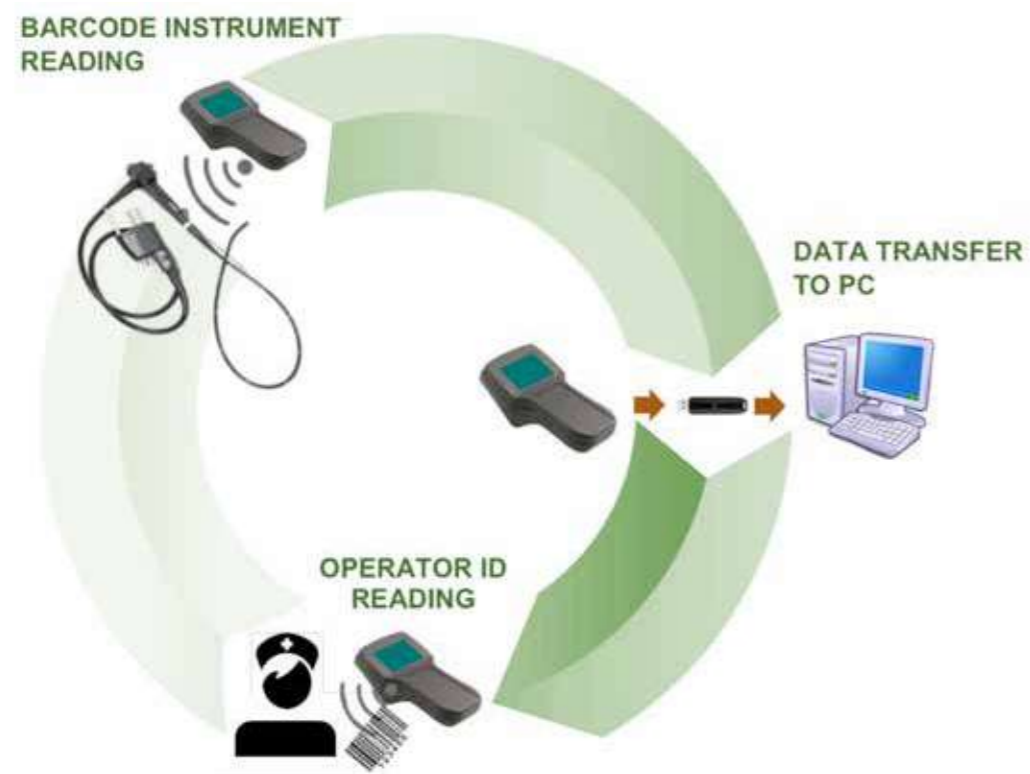

MEDICAL DEVICES GROUP Srl
Via G.Fracastoro, 1 48124 Ravenna (RA)
Tel +39 0544 1826013
Fax +39 0544 1826015
www.mdg-srl.com - info@mdg-srl.com



Complies with the Directive 93/42/CEE Annex VII

giantucalerrini.com
Vers. 1/2018

LT-217[®]

tester to check integrity of flexible endoscopes

+
For all types of flexible endoscopes
mdg - patent



DATA TRANSFER
through USB flash drive



DISPLAY LCD
backlit LCD display



CONNECTORS
Instrument connectors for each brand



AUTOMATIC RECOGNITION
it recognizes automatically the instrument



INTERGRATED BAR CODE
to read operator an instrument ID



+
LT-217®
To check endoscope channels, sheaths and o'ring conditions

+
Italian technology and design



LT-217®

tester to check integrity of flexible endoscopes

LT-217® is a patented system designed to check the integrity of flexible endoscopes. The device detects accurately leakage of the sheaths, of the endoscopes channels and the wear conditions of the o'ring.

It checks also the conditions of internal channels and the little holes caused by twisted biopsy channels. This leak tester works through much higher standard compared to the actual product on the market and because of this it drastically reduces infiltrations during endoscope reprocessing procedures.

LT-217® is a MDG s.r.l. patent.

Standard equipment:

- Power supply for internal batteries
- Connection hose
- Leak test connector
- End-user and maintenance manual
- Flash drive cable to download the stored cycles.